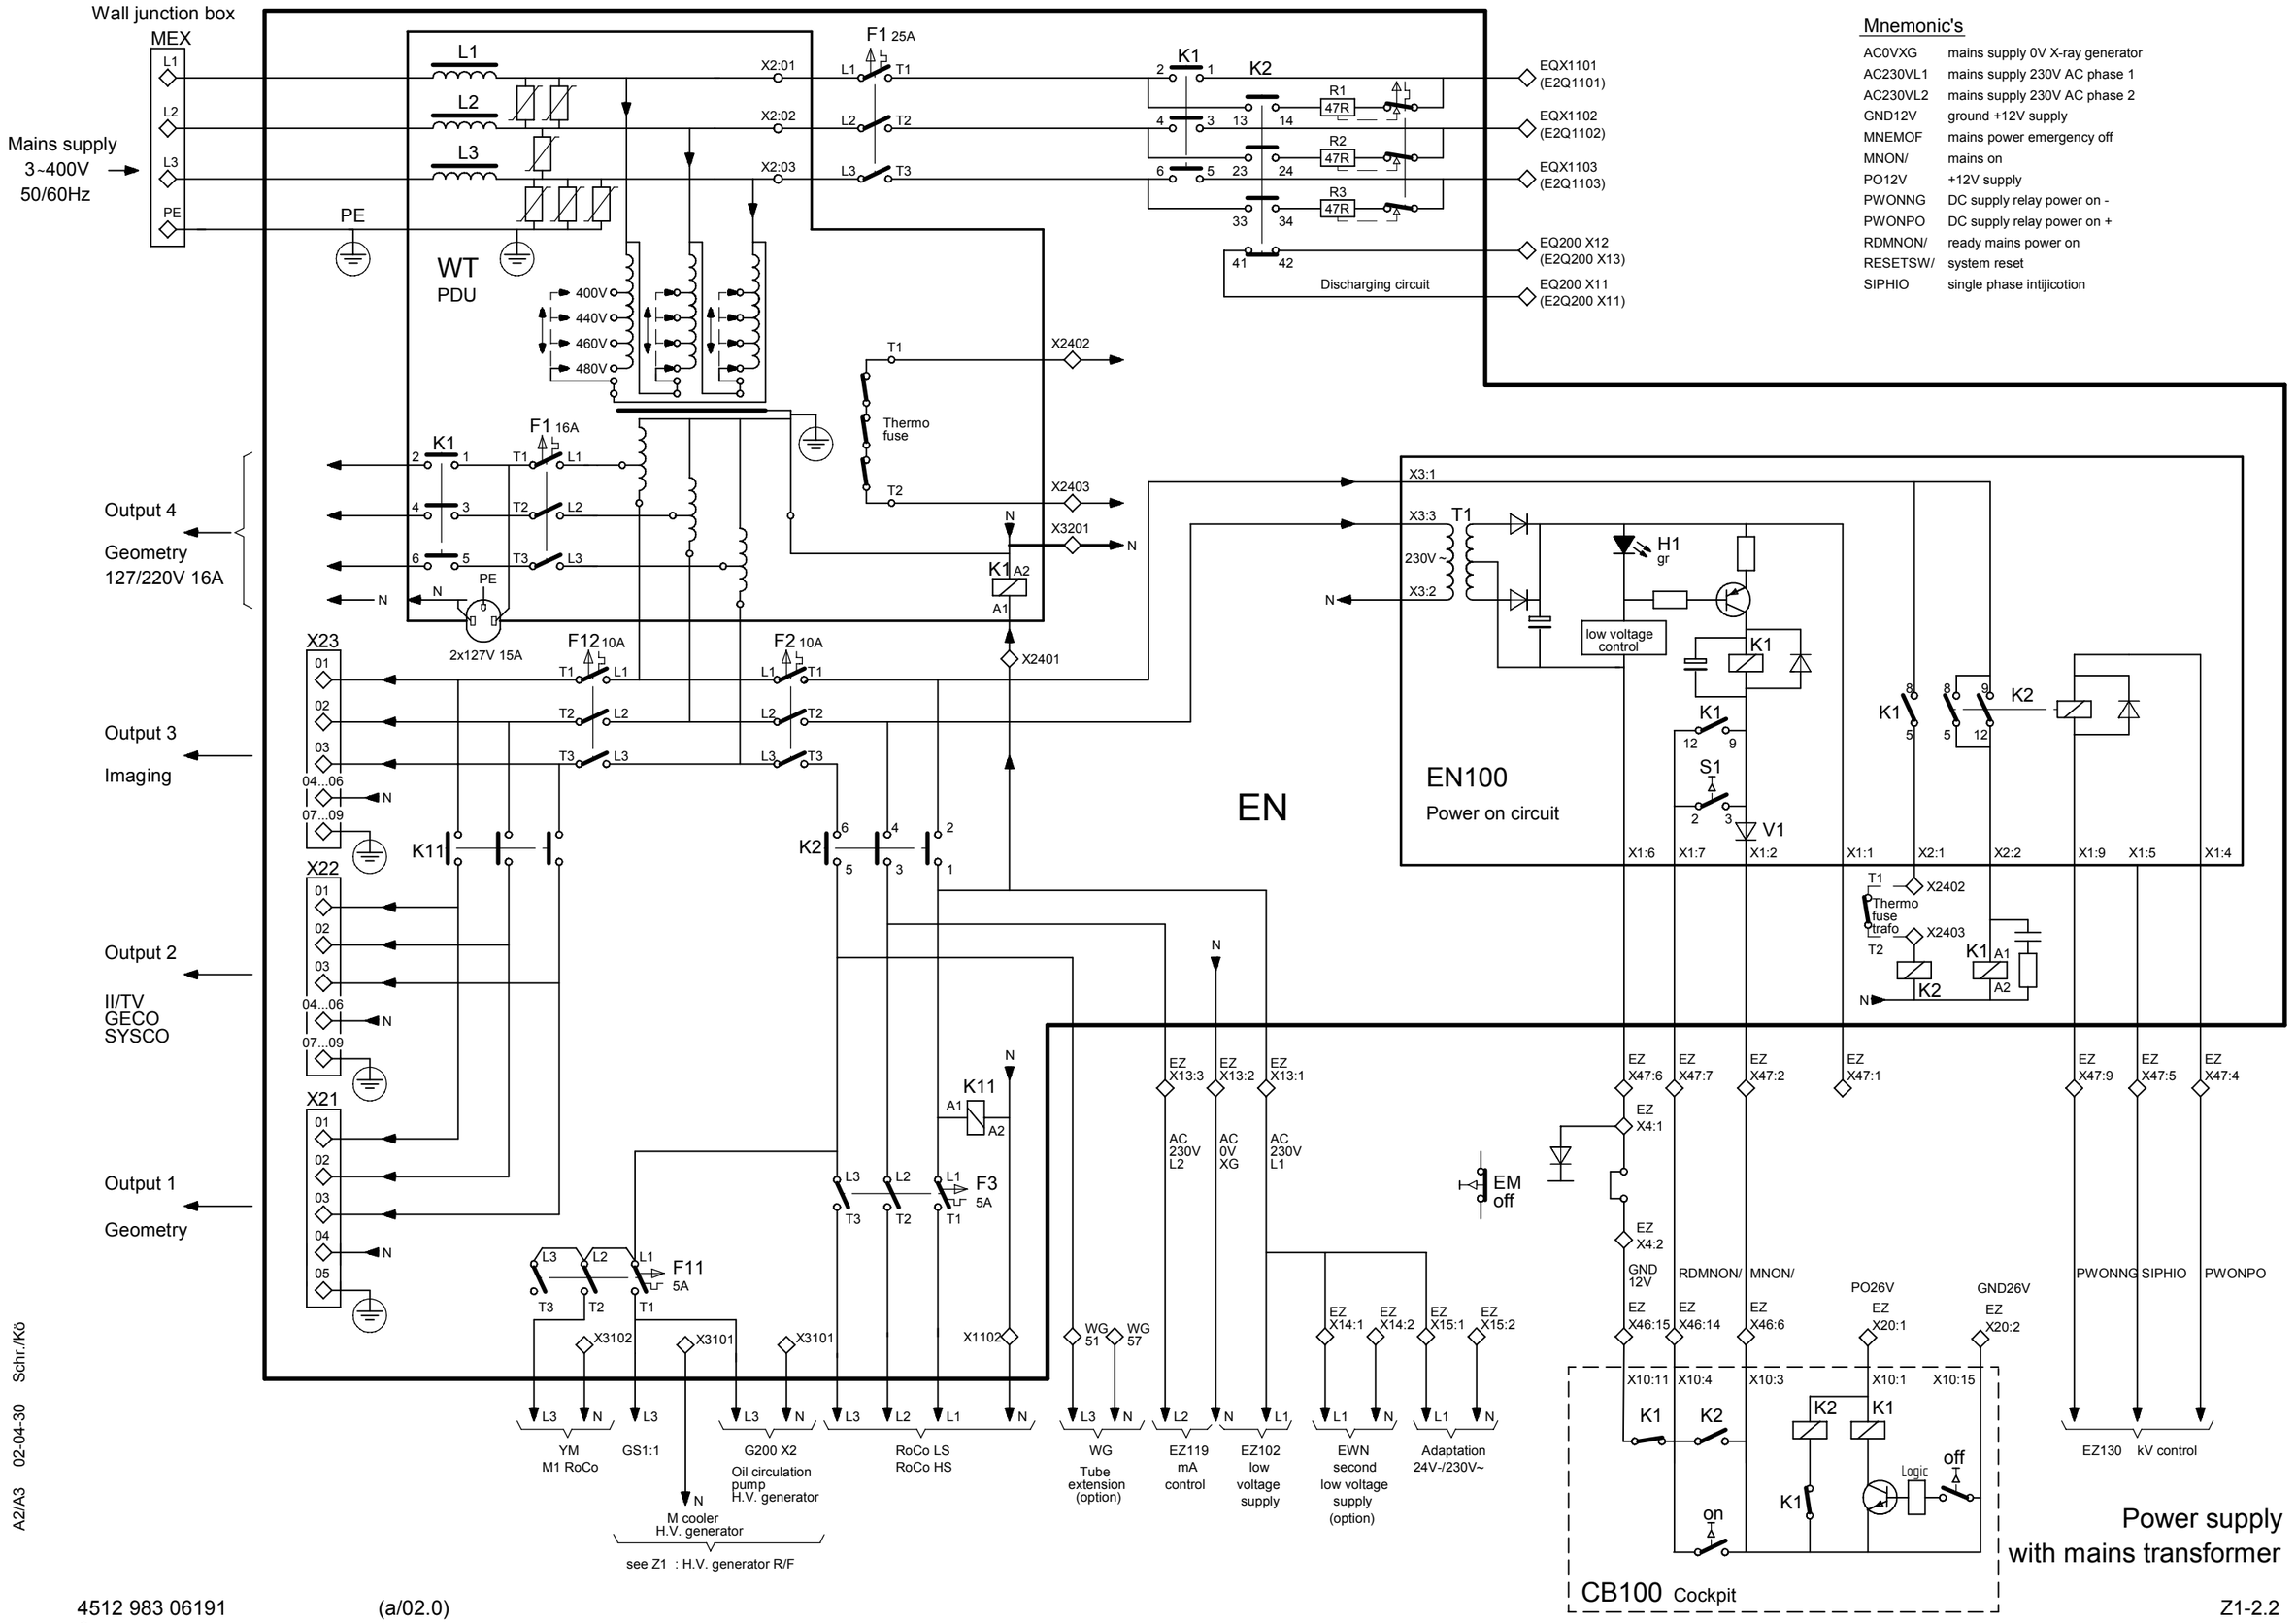


Mnemonic's

| | |
|---|---|
| AC0VXG | mains supply 0V X-ray generator |
| AC230VL1 | mains supply 230V AC phase 1 |
| AC230VL2 | mains supply 230V AC phase 2 |
| GND12V | ground +12V supply |
| MNEMOF | mains power emergency off |
| MNON/ | mains on |
| PO12V | +12V supply |
| PWONNG | DC supply relay power on - |
| PWONPO | DC supply relay power on + |
| RDMNON/ | ready mains power on |
| RESETSW/ | system reset |
| SIPHIO | single phase intjicotion |

A2/A3 02-04-30 Schr./Kö

4512 983 06191 (a/02.0)

© Philips Medical Systems